

**FIG. 1**

**Needle Penetration Test by Rheometer**

Immersion time 0 hrs

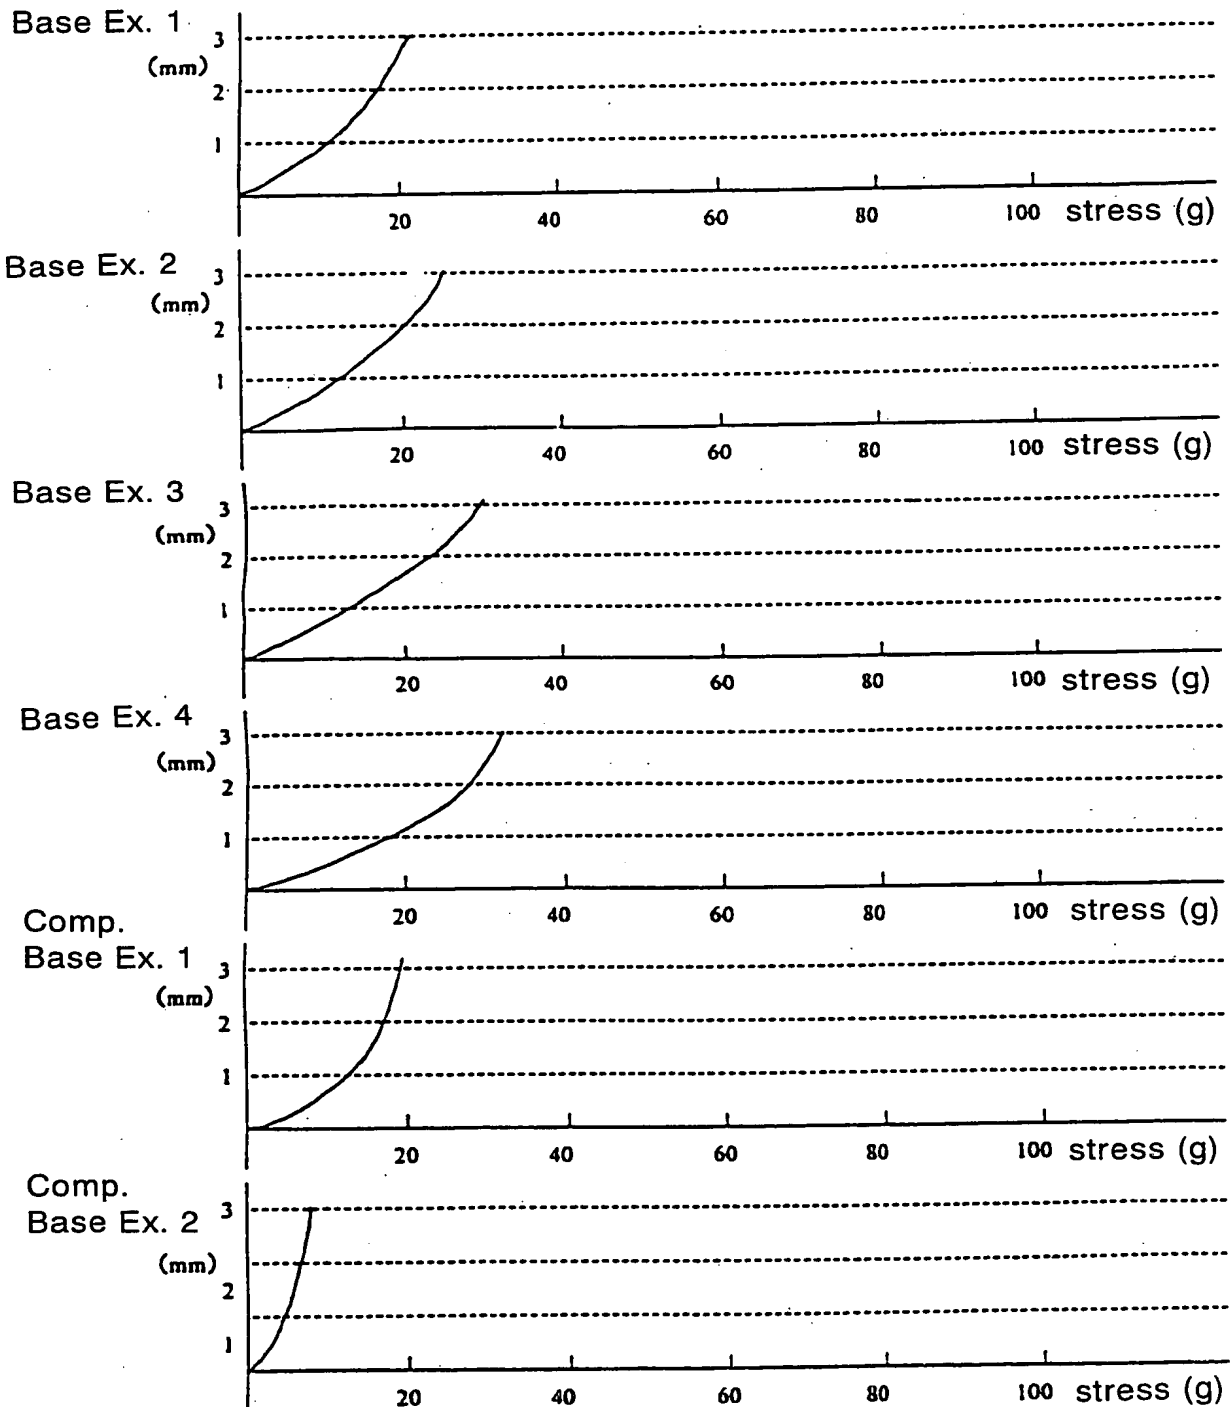
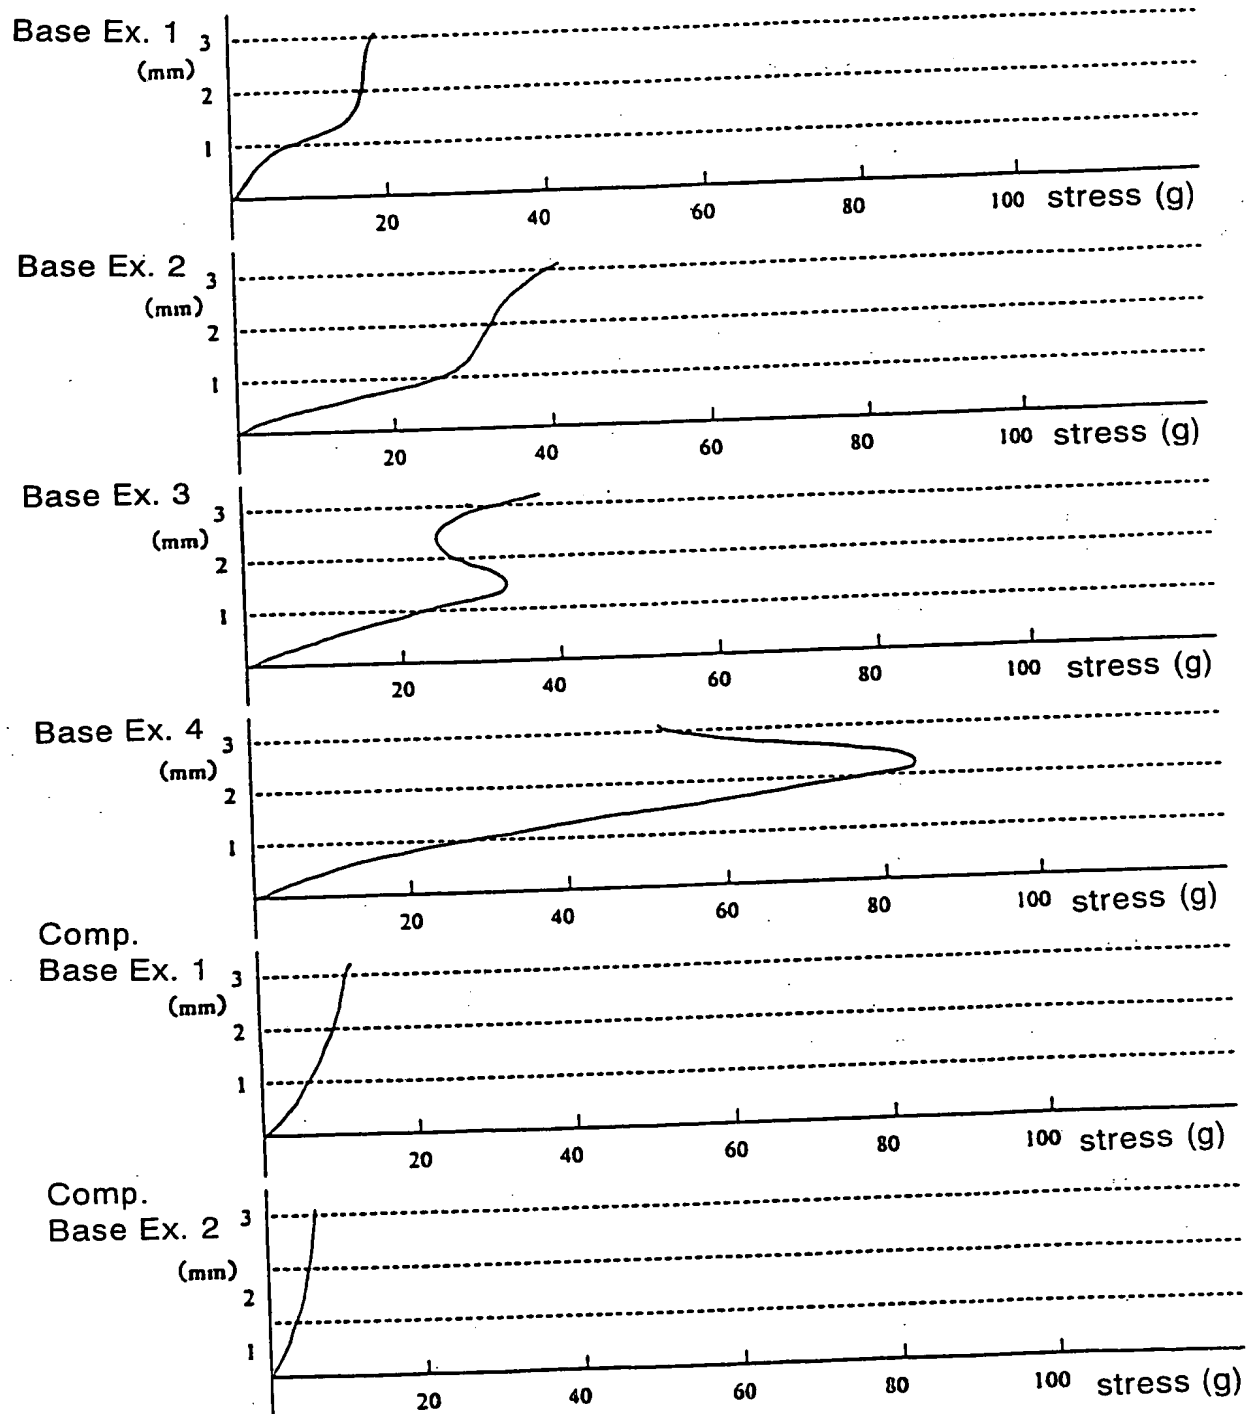


FIG. 2

Needle Penetration Test by Rheometer

Immersion time 24 hrs



**FIG. 3**

Needle Penetration Test by Rheometer

Immersion time 48 hrs

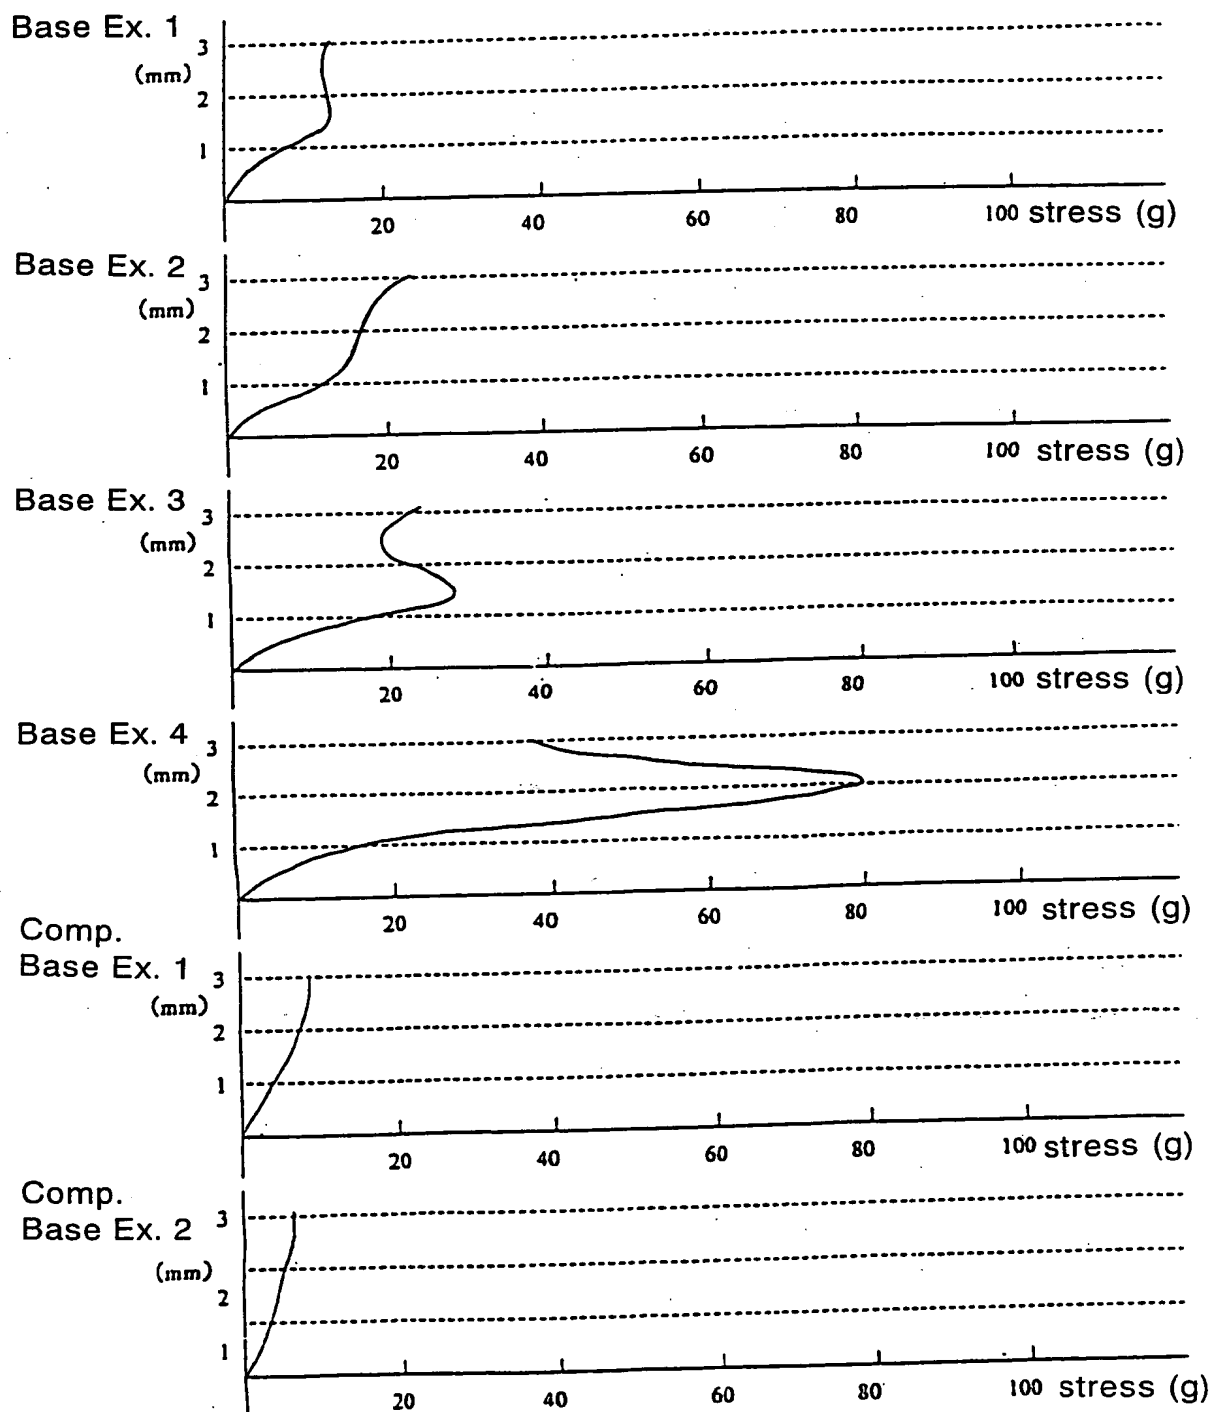


FIG. 4

